



中国认可
国际互认
检测
TESTING
CNAS L1842

FCL
No.002



佛山中纺联检验技术服务有限公司
CNTAC Testing Service Co.,Ltd.(Foshan)

Testing Report	Security website: www.fcl-sz.org.cn Security code: 1555712052
Report No: ZFLJ2634914A	Page 1 of 3



Applicant Information

Applicant Name : Anqing Rixin Sanitary Material Co., Ltd
Applicant Address : Huaining Industrial Park, Anqing City, Anhui Province

Sample Information

Sample Description : Disposable protective mask(child type)
Sample Quantity : 35 pieces

- Sample Receiving Date : 2020-07-08
- Report Date : 2020-07-13
- The original sample is stuck on the last paper.

Test Performed

Judgement according to:
GB/T 38880-2020 Technical specification of children mask Children protective mask
- Selected test(s) as requested by applicants. For details, refer to attached page(s).

Pronounce

The results shown in this report refer only to sample(s) tested unless otherwise stated.
All the items are performed in the standard conditions, except the noted cases.
Except for the requirement of the client, the test results and the conformity judgement of this report do not take the uncertainty of the test results into account.

Signed for and on behalf of
CNTAC Testing Service Co.,Ltd.(Foshan)

Approved by

张志荣





中国认可
国际互认
检测
TESTING
CNAS L1842

FCL
No.002



佛山中纺联检验技术服务有限公司
CNTAC Testing Service Co.,Ltd.(Foshan)

Testing Report	Security website: www.fcl-sz.org.cn Security code: 1555712052
Report No: ZFLJ2634914A	Page 2 of 3



--- Test Result ---

Test Result	Requirements	Judgement
1. Tensile Strength of the mask belt and the connection between the mask belt and the mask body <u>GB/T 32610-2016 Section 6.9</u> Unit: <N>		
Result	25	≥ 15
		Pass
2. pH Value <u>GB/T 7573-2009</u> Using KCl solution as the extracting solution.		
Result	6.2	4.0~7.5
		Pass
3. Formaldehyde Content <u>GB/T 2912.1-2009</u> Water extraction method, lower limit of quantitation: 20mg/kg Unit: <mg/kg>		
Result	Not Detectable	≤ 20
Remark: Not Detectable, Less than 20 mg/kg		Pass
4. Particle Filtration Efficiency <u>GB/T 32610-2016 Appendix A</u> Air flow: 85L/min, Aerosol: NaCl. Unit: <%>		
Before pretreatment		≥ 95
sample 1#	96.2	
sample 2#	97.1	
sample 3#	96.1	
sample 4#	97.0	
sample 5#	98.0	
After pretreatment		
sample 1#	96.2	
sample 2#	96.4	
sample 3#	97.0	
sample 4#	96.7	
sample 5#	96.3	
Minimum value	96.1	





中国认可
国际互认
检测
TESTING
CNAS L1842



佛山中纺联检验技术服务有限公司
CNTAC Testing Service Co.,Ltd.(Foshan)

Testing Report


Security website: www.fcl-sz.org.cn
Security code: 1555712052



Report No: ZFLJ2634914A

Page 3 of 3

Original Sample

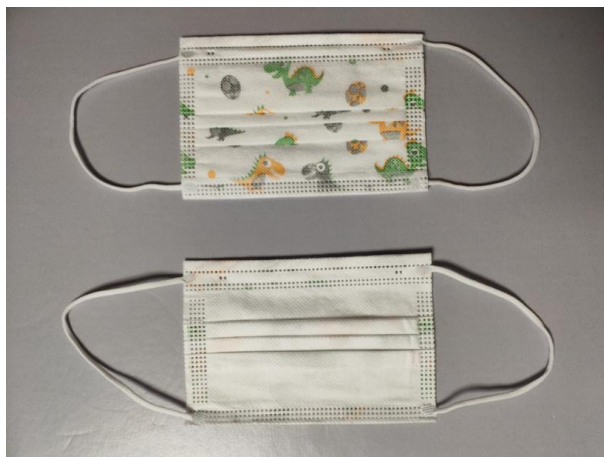

===== End of Report =====

